SpeedBand SuperView Super 7™

Multiple Band Ligator


Boston Scientific




Attach Handle Unit to Endoscope

1- Step One Straighten endoscope

Feed trip wire through working channel **3- Step Three** Insert handle unit into biopsy valve **4- Step Four** Secure handle to endoscope with strap



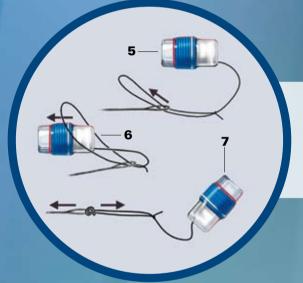

Attach Ligating Unit to Trip Wire

Thread pulling loop through trip wire loop Thread ligating unit through pulling loop 6- Step Six

7- Step Seven Pull to tighten

Attach Ligating Unit to Endoscope

8- Step Eight Grasp trip wire loop at handle and retract until ligating unit contacts tip of endoscope

9- Step Nine Align black stripe with working channel and push ligating unit onto

DO NOT TAKE UP TRIP WIRE SLACK BY ROTATING







Complete Preparation for Use

10- Step Ten Grasp trip wire and retract to remove slack, then lock down by pulling across

narrow slot

DO NOT OVER TIGHTEN

11- Step Eleven Carefully remove shrink wrap by hand

12- Step Twelve OPTIONAL: Attach irrigation tube

Scientific

Delivering what's next.™

RCS Nanterre B420 668 420 © 2007 Boston Scientific Corporation or its affiliates. All rights reserved. DIN**END**2168EB

^{*}This overview is provided for illustrative purposes only and is intended only as a brief summary of how the set-up procedures for the SpeedBand SuperView Super 7 are generally performed. Please refer to the Directions For Use for complete set-up instructions and precautions. NOTE: Designed to fit on scopes with outer diameter of 8.6–11.5mm.

All cited trademarks are the property of their respective owners. CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable